

इंटरनेट

मानक

Disclosure to Promote the Right To Information

Whereas the Parliament of India has set out to provide a practical regime of right to information for citizens to secure access to information under the control of public authorities, in order to promote transparency and accountability in the working of every public authority, and whereas the attached publication of the Bureau of Indian Standards is of particular interest to the public, particularly disadvantaged communities and those engaged in the pursuit of education and knowledge, the attached public safety standard is made available to promote the timely dissemination of this information in an accurate manner to the public.

“जानने का अधिकार, जीने का अधिकार”

Mazdoor Kisan Shakti Sangathan

“The Right to Information, The Right to Live”

“पुराने को छोड़ नये के तरफ”

Jawaharlal Nehru

“Step Out From the Old to the New”

IS 12872 (2011): Metallic Materials – Calibration of Extensometers Used in Uniaxial Testing [MTD 3: Mechanical Testing of Metals]



“ज्ञान से एक नये भारत का निर्माण”

Satyanarayan Gangaram Pitroda

“Invent a New India Using Knowledge”



“ज्ञान एक ऐसा खजाना है जो कभी चुराया नहीं जा सकता है”

Bhartrhari—Nitiśatakam

“Knowledge is such a treasure which cannot be stolen”

BLANK PAGE



IS 12872 : 1990

ISO 9513 : 1989

(Reaffirmed 2006)

Indian Standard

**METALLIC MATERIALS — VERIFICATION OF
EXTENSOMETERS USED IN UNIAXIAL TESTING**

भारतीय मानक
धात्विक सामग्री — एकाक्ष परीक्षण में प्रयुक्त
एक्सटेन्सोमीटरों का सत्यापन

UDC 620.172.2.087.45:53.089.6

© BIS 1990

BUREAU OF INDIAN STANDARDS
MANAK BHAVAN, 9 BAHADUR SHAH ZAFAR MARG
NEW DELHI 110002

August 1990

Price Group 4

Indian Standard

**METALLIC MATERIALS — VERIFICATION OF
EXTENSOMETERS USED IN UNIAXIAL TESTING**

NATIONAL FOREWORD

This Indian Standard, which is identical with ISO 9513:1989 'Metallic materials — Verification of extensometers used in uniaxial testing', issued by the International Organization for Standardization (ISO), was adopted by the Bureau of Indian Standards on 20 April 1990 on the recommendation of the Mechanical Testing of Metals Sectional Committee (MTD 3) and approval of the Metallurgical Engineering Division Council.

In the adopted standard certain conventions are not identical with those used in Indian Standards. Attention is specially drawn to the following:

- a) Wherever the words 'International Standard' appear referring to this standard, they should be read as 'Indian Standard'.
- b) Comma (,) has been used as a decimal marker while in Indian Standards the current practice is to use point (.) as the decimal marker.

As in the Original Standard, this Page is Intentionally Left Blank

1 Scope

This International Standard specifies a method for the static verification of extensometers used in uniaxial testing.

The term "extensometer" is understood to mean the displacement measuring device and the system for indicating or recording this displacement.

2 Symbols and their meanings

Symbols used throughout this International Standard and their meanings are given in table 1.

Table 1 — Symbols and their meanings

Symbol	Meaning	Unit
L_e	Nominal value of gauge length of extensometer	mm
L'_e	Measured value of gauge length of extensometer	mm
E_{max}	Maximum limit of verification range	mm
E_{min}	Minimum limit of verification range	mm
l_i	Displacement indicated by extensometer	μm
l_t	True displacement given by calibration apparatus	μm
q_{Le}	Relative gauge length error	%
q	Relative bias error of extensometer	%
r	Resolution of extensometer	μm

3 Principle

The verification of an extensometer involves a comparison of the readings given by the extensometer with known variations in length provided by a calibration apparatus.

4 Calibration apparatus

The calibration apparatus which allows a known displacement, l_t , to be applied to the extensometer may consist of a rigid frame with suitable coaxial spindles or other fixtures to which the extensometer can be attached. The calibration apparatus shall comprise a mechanism for moving at least one of the axial

spindles and a device for measuring accurately the change in length produced. The variations in length can be measured, for example, using an interferometer or gauge blocks and a comparator or a screw micrometer. The gauge blocks and comparator or micrometer used shall be calibrated by a method which is traceable to the international unit (SI) of length and their accuracy shall be known. The error of the calibration apparatus shall not be greater than one-third of the permissible error of the extensometer (see table 2).

The resolution of the calibration apparatus shall be as given in table 2.

5 Procedure

5.1 Position of the extensometer

The extensometer shall be placed in the calibration apparatus in the same position and orientation in which it is used during uniaxial testing so as to avoid errors due to loss of equilibrium or deformation of any part of the extensometer.

The extensometer shall be attached in the same way as during uniaxial testing.

5.2 Temperature at which the verification is made

In general, the verification of the extensometer shall be carried out at a temperature stable to within $\pm 2^\circ\text{C}$; this temperature shall be within the range between 18°C and 28°C .

For extensometers used for uniaxial testing at temperatures outside the range specified above, it is recommended that the verification be carried out at or near the test temperature, if facilities exist.

The extensometer shall be placed near the calibration apparatus or mounted on it for a sufficient length of time prior to its verification so that the parts of the extensometer and of the calibration apparatus which are in contact shall attain the same temperature.

5.3 Accuracy of gauge length of the extensometer

The gauge length of the extensometer can be measured directly or indirectly. The following indirect method is given as an example.

The extensometer is placed on a soft metal test piece in such a way that the blades or points of the extensometer leave their mark. Once the extensometer is removed, the distance between the marks on the test piece is measured.

The relative error on the gauge length, q_{L_e} , calculated from the following formula shall not exceed the values given in table 2 :

$$\frac{L'_e - L_e}{L_e} \times 100$$

In the case of an extensometer having several gauge lengths, the verification shall be carried out for each gauge length.

5.4 Range of verification

The verification range shall be defined by the user to cover the measuring range required to determine a given material property. The maximum and minimum limits $E_{\max}$ and $E_{\min}$ of the verification range shall be such that

$$\frac{E_{\max}}{E_{\min}} < 10$$

If several ranges are specified by the user, each one shall be verified. An example of verification ranges is given in annex A. The ranges of verification shall be noted in the verification report.

5.5 Verification procedure

5.5.1 When the temperature has stabilized, it is recommended that, before verification, the extensometer be extended at least twice by the verification apparatus over the verification range of the extensometer. If possible, the displacement is taken to a slightly negative value and returned to zero. Where appropriate, the extensometer is reset to zero.

5.5.2 The verification consists first of one series of at least 10 measurements, l_i , distributed approximately evenly throughout the verification range of the extensometer. The extensometer is removed and then placed back on the calibration apparatus. A second series of measurements is then made in the same manner as the first. For each series of measurements the successive variations in length shall be of the same type (i.e. either increases or decreases).

Depending on the expected use of the extensometer, the two series of measurements are made for increases in length or for decreases in length or for both.

For each measurement point, the relative bias error is calculated (see 5.6.2).

5.6 Determination of the characteristics of the extensometer

5.6.1 Resolution

The resolution, r , is the smallest quantity which can be read on the instrument. The values of the resolution of the extensometer shall be in accordance with the values given in table 2.

5.6.2 Relative bias error

The relative bias error, q , for a given displacement, l_i is calculated from the formula

$$\frac{l_i - l_t}{l_t} \times 100$$

6 Classification of the extensometer

Table 2 gives the maximum permissible values for the relative gauge length error, the resolution and the relative bias error.

Table 2 — Classification of extensometers

Class of extensometer	Extensometer					Calibration apparatus (Maximum values)	
	Maximum relative error on the gauge length q_{L_e} %	Resolution ¹⁾		Bias ¹⁾		Resolution μm	Absolute bias error μm
		Maximum percentage of reading r/l_i %	Maximum absolute value r μm	Maximum relative error q %	Maximum absolute error $l_i - l_t$ μm		
0,5	± 0,5	0,25	± 0,5	± 0,5	± 1,5	0,25	± 0,5
1	± 1,0	0,50	± 1,0	± 1,0	± 3,0	0,50	± 1,0
2	± 2,0	1,0	± 2,0	± 2,0	± 6,0	1,0	± 2,0

1) Whichever value is the greater.

7 Frequency of verification

The time between two verifications depends on the type of extensometer, the maintenance standard and the number of times the extensometer has been used. Under normal conditions, it is recommended that verification be carried out at intervals of approximately 12 months. In no case shall the interval exceed 18 months.

If a test is expected to last more than 18 months, the extensometer shall be verified before and after the test.

The extensometer shall be verified if it undergoes any major repairs or adjustments.

8 Verification report

The verification report shall contain at least the following information :

a) General information :

- 1) reference to this International Standard;

- 2) identification of the extensometer (type, make, serial number and mounting position);

- 3) type and reference number of calibration apparatus;

- 4) temperature at which the verification was carried out;

- 5) nature of variations of length for which the verification was carried out, i.e. either for increases and/or for decreases in length;

- 6) date of verification;

- 7) name or mark of the service which carried out the verification;

- 8) date of expiry of the verification report.


b) Results of the verification :

- 1) class of each range of the extensometer;

- 2) the individual values of the relative bias errors, if requested.

Annex A
(informative)

Example of verification ranges of an extensometer

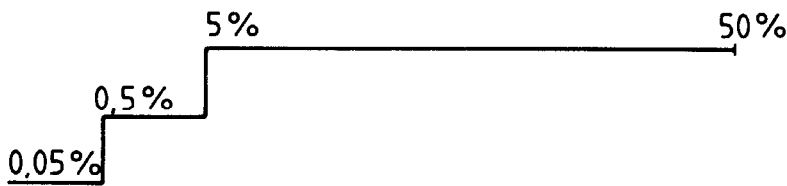

First verification range :	0,05 % to 0,5 %	} of the nominal value of the extensometer travel
Second verification range :	0,5 % to 5 %	
Third verification range :	5 % to 50 %	

Annex B (informative)

Parameters for classification of an extensometer

In order to clarify the definition of the parameters used for the classification of an extensometer in accordance with clause 6

- table B.1 gives three examples of calculations of these parameters;
- the diagrams in figures B.1 and B.2 illustrate clearly, for class 1 extensometers, how to decide which of the two limits, "relative" or "absolute", should be chosen.

Table B.1 — Examples of calculation of parameters for the classification of extensometers

Gauge length of the extensometer l_e mm	True value		Measured value		Error		Relative bias error ¹⁾ , q (%)	
	Displacement l_t μm	Deformation $l_t/l_e = e_t$	Displacement l_i μm	Deformation $l_i/l_e = e_i$	Displacement $l_i - l_t$ μm	Deformation $e_i - e_t$	Displacement $\frac{l_i - l_t}{l_t} \times 100$	Deformation $\frac{e_i - e_t}{e_t} \times 100$
50	100	2×10^{-3}	110	$2,2 \times 10^{-3}$	10	$0,2 \times 10^{-3}$	10	10
100	100	1×10^{-3}	110	$1,1 \times 10^{-3}$	10	$0,1 \times 10^{-3}$	10	10
100	200	2×10^{-3}	210	$2,1 \times 10^{-3}$	10	$0,1 \times 10^{-3}$	5	5

1) For a given displacement error, the relative error, q , is independent of the gauge length of the extensometer, l_e , but is dependent on the displacement value, l_t .

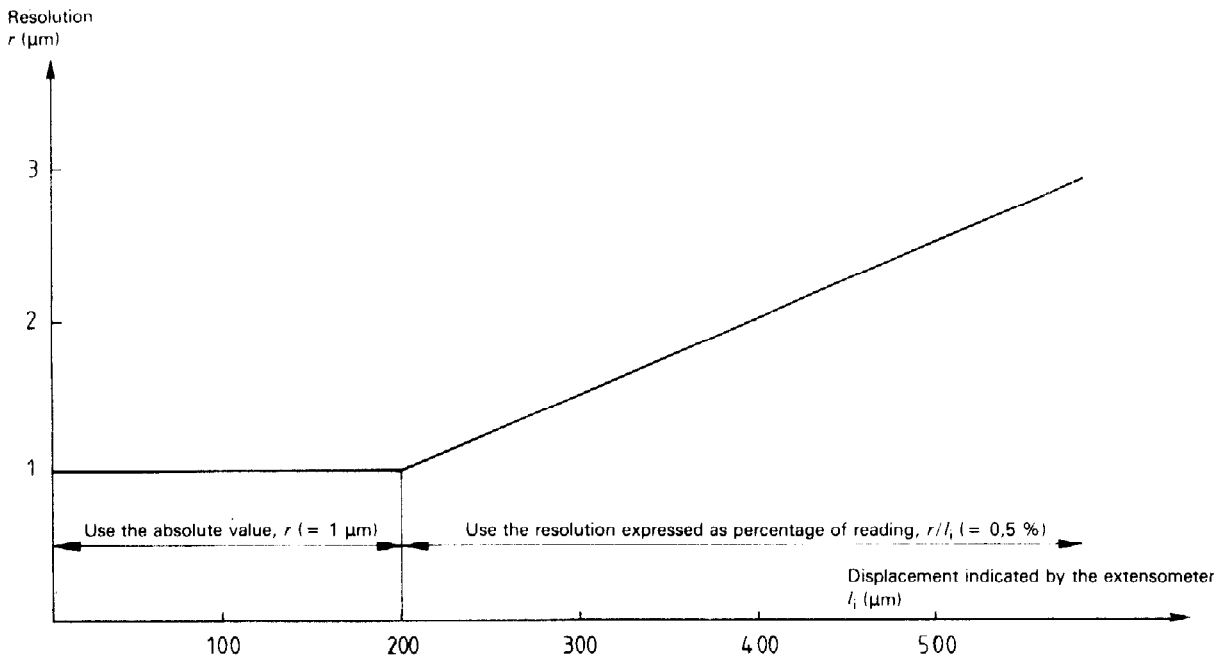


Figure B.1 — Resolution of a class 1 extensometer

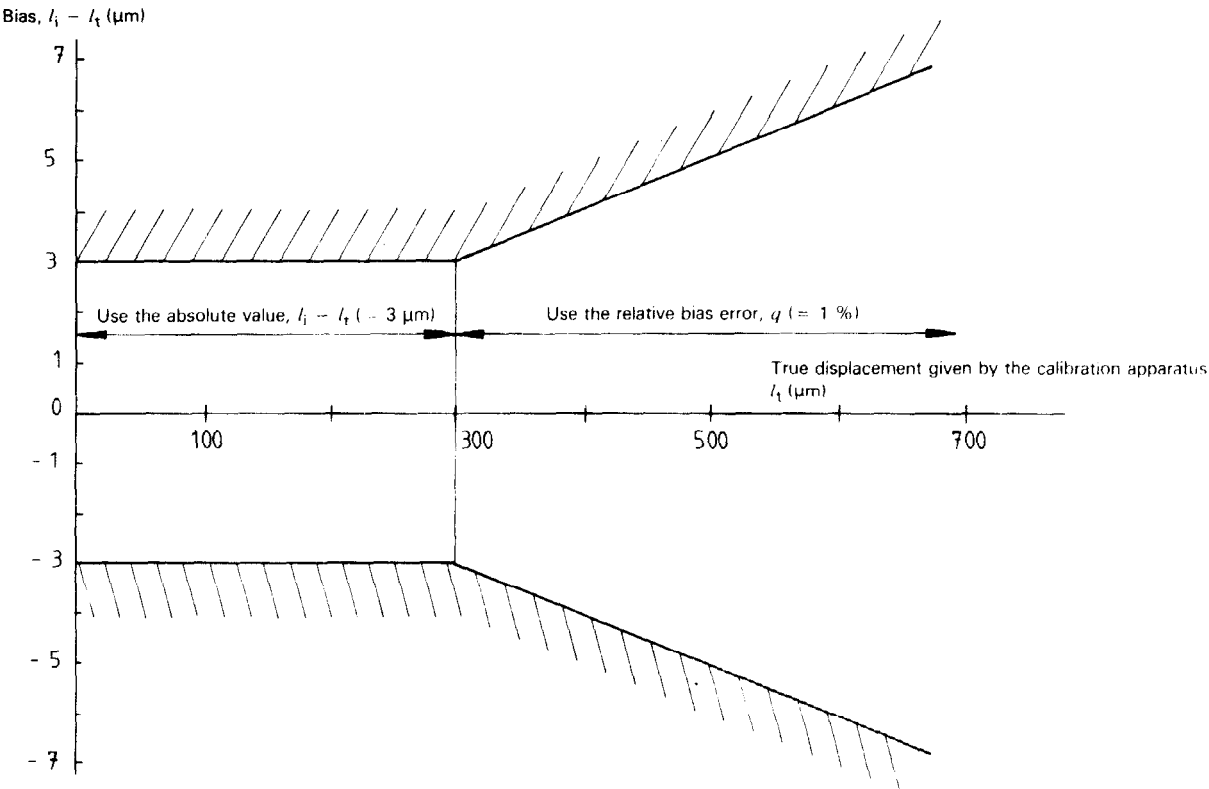


Figure B.2 — Limits of bias error of a class 1 extensometer

Bureau of Indian Standards

BIS is a statutory institution established under the *Bureau of Indian Standards Act, 1986* to promote harmonious development of the activities of standardization, marking and quality certification of goods and attending to connected matters in the country.

Copyright

BIS has the copyright of all its publications. No part of these publications may be reproduced in any form without the prior permission in writing of BIS. This does not preclude the free use, in the course of implementing the standard, of necessary details, such as symbols and sizes, type or grade designations. Enquiries relating to copyright be addressed to the Director (Publications), BIS.

Revision of Indian Standards

Indian Standards are reviewed periodically and revised, when necessary and amendments, if any, are issued from time to time. Users of Indian Standards should ascertain that they are in possession of the latest amendments or edition. Comments on this Indian Standard may be sent to BIS giving the following reference:

Doc. No. MTD 3 (3462)

Amendments Issued Since Publication

Amend No.	Date of Issue	Text Affected

BUREAU OF INDIAN STANDARDS

Headquarters :

Manak Bhavan, 9 Bahadur Shah Zafar Marg, New Delhi 110002
Telephones : 331 01 31, 331 13 75

Telegrams : Manaksanstha
(Common to all Offices)

Regional Offices :

Central : Manak Bhavan, 9 Bahadur Shah Zafar Marg
NEW DELHI 110002

Telephone

{ 331 01 31
331 13 75

Eastern : 1/14 C. I. T. Scheme VII M, V. I. P. Road, Maniktola
CALCUTTA 700054

37 86 62

Northern : SCO 445-446, Sector 35-C, CHANDIGARH 160036

2 18 49

Southern : C. I. T. Campus, IV Cross Road, MADRAS 600113

41 29 16

Western : Manakalaya, E9 MIDC, Marol, Andheri East)
BOMBAY 400093

6 32 92 95

Branches : AHMADABAD. BANGALORE. BHOPAL. BHUBANESWAR.
COIMBATORE. FARIDABAD. GHAZIABAD. GUWAHATI.
HYDERABAD. JAIPUR. KANPUR. PATNA. TRIVANDRUM.